



Parameters

Operation mode:	Seven working modes
Brightness :	Adjustable(four levels)
Light source:	Near-infrared light
Net weight :	350g
Dimension :	228mm*63mm*62mm
Battery standby time:	≤ 4.5h
Optimal imaging distance :	210mm±30mm

Projection Vein Finder reduces the first venipuncture failure rate by 77. 5%, and the infiltration rate by 61. 4%.

——Clinical data from a comparative study of 360 cases. The results of this study had been published on Journal of Nursing Administration, September 2015.



Shenzhen Vivolight Medical Device & Technology Co.,Ltd.

Manufacturer Add: Rm. 201-2, Building 1, Liu Xiandong SCI & TECH Park, Nanshan District, 518055 Shenzhen, China
Office Add: F2-4B, International E city of TCL Science Park,Zhongshanyuan Road, Nanshan District, Shenzhen, China
Web: www.vivo-light.com Tel: +86(0)755 8696 1139 Email: sales@vivo-light.com

Accurate/Efficient/Portable/Safe

Projection
Vein
Finder

V800P

PROJECTION VEIN FINDER



New
features




Photo



Storage

Principle


The Projection Vein Finder V800P is based on the principle that human hemoglobin has a higher absorption of infrared light than other tissues. With our enhanced imaging processing unit, up to 80% invisible veins can be detected. The processed vein image is synchronously and precisely projected back on to the skin.

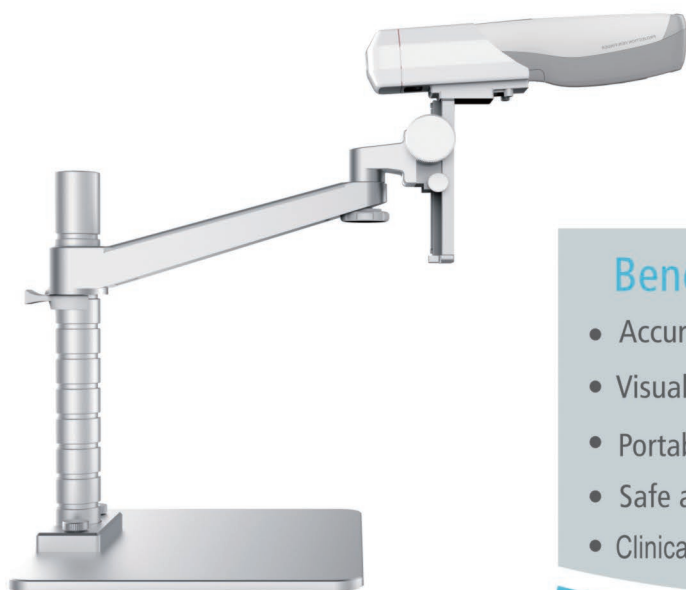


Benefits

- Accurate Alignment accuracy $\leq 0.5\text{mm}$
- Visualized DLP real-time in situ display
- Portable Compact and convenient
- Safe adopt Near infrared light
- Clinical evidence Image capture & saving

Different Modes:

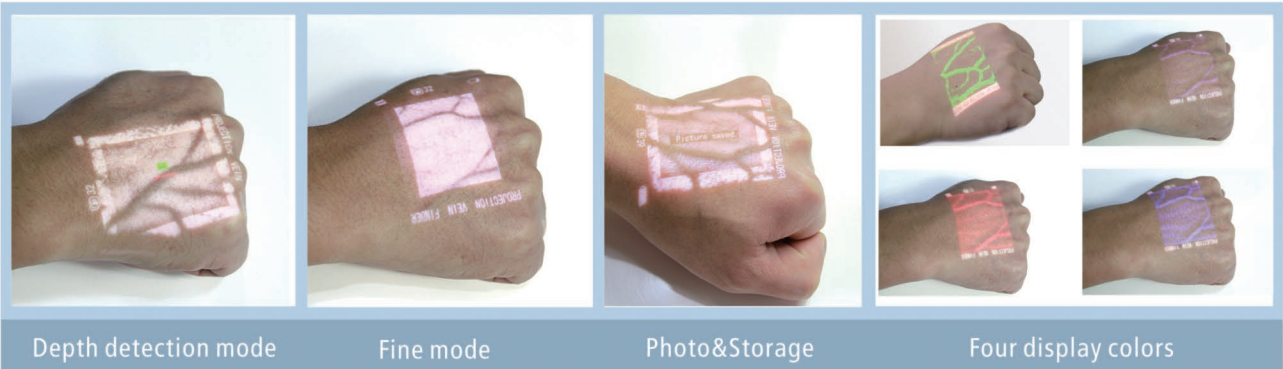

Different Parts:

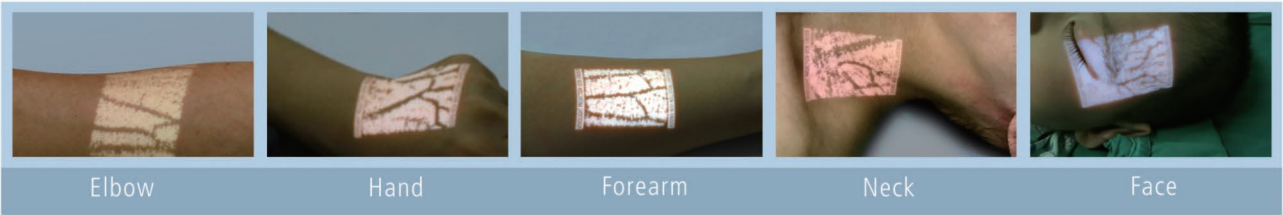

Highly recommended by INS Infusion therapy standard practice

- 22.1 To ensure patient safety, the clinician is competent in the use of vascular visualization technology for vascular access device (VAD) insertion. This knowledge includes, but is not limited to, appropriate vessels, size, depth, location, and potential complications.
- 22.2 Vascular visualization technology is used in patients with difficult venous access and/or after failed venipuncture attempts.
- 22.3 Vascular visualization technology is employed to increase the success with peripheral cannulation and decrease the need for central vascular access device (CVAD) insertion, when other factors do not require a CVAD.

- Features :** Depth detection
Various display colors
Adjustable brightness

Clinical Application

